



طرح عطاء مدفوع

يعلن مستشفى النجاح الوطني الجامعي عن طرح عطاء رقم RFQ-H-11478 والخاص بشراء أجهزة طبية ، على الشركات المتخصصة والراغبة بالمشاركة بالعطاء تقديم عروض اسعارها في موعد أقصاه يوم الخميس الموافق 10/03/2022 الساعة الواحدة ظهراً PM 13:00 وفقاً للاتى:

وقت الإغلاق	التاريخ	موعد الطرح	ثمن نسخة العطاء	موضوع العطاء	رقم العطاء	#
الساعة						
P.M 13:00	2022/03/10	2022/01/24	250 شيكل غير مستردة	اجهزة طبية	RFQ-H-11478	1

حسب الشروط التالية:

1. ضرورة ارفاق الرخصة التجارية والسيرة الذاتية للشركة مع عرض السعر .
2. رسوم الاعلان على من يرسو عليه العطاء .
3. ثمن نسخة العطاء 250 شيكل غير مستردة .
4. كغالة دخول عطاء بقيمة (1000) الف دولار أمريكي .

على الراغبين بالاشتراك في العطاء المذكور طلبه بواسطة ارسال رسالة على الايمل التالي [tender3@najah.edu](mailto:tender3@najah.edu) او مراجعة دائرة اللوازم والمشتريات مكتب رقم 6400 \ في مستشفى النجاح الوطني الجامعي مبنى الإدارة ، للحصول على نسخة من وثائق العطاء .

للاستفسار يرجى الاتصال على :

دائرة اللوازم والمشتريات في مستشفى النجاح الوطني الجامعي – البريد الالكتروني [tender3@najah.edu](mailto:tender3@najah.edu) هاتف +970-09-2331471 فاكس: +970-9-2389685 .

التاريخ : 24/02/2022

**طرح عطاء رقم – RFQ-H-11478**

السادة / الشركات المختصة الراغبة بالمشاركة بالعطاء - المحترمين .


الموضوع : أجهزة طبية ، حسب المواصفات المرفقة .

بالإشارة إلى الموضوع أعلاه، يرجى الاطلاع على جداول المواصفات المرفقة مع مراعاة الشروط التالية :-

1. تكتب الاسعار بالشكل الاسرائيلي وبشكل واضح في المكان المخصص حسب الجدول المرفق وتشمل قيمة الضريبة المضافة، في حال وجود تعارض بين سعر الوحدة ومجموع سعر الوحدة المشتق، فإن سعر الوحدة هو الذي سيعتمد .
2. ثمن نسخة العطاء (250) شيكل إسرائيلي غير مستردة تدفع في الدائرة المالية مبنى الإدارة - الطابق الأول .
3. كفالة دخول عطاء بقيمة (1000) ألف دولار امريكي او ما يعادلها سارية المفعول لمدة ثلاثة شهور تأميناً نقدياً او كفالة بنكية او شيكاً مصدقاً وفي حالة عدم تقديم التأمين لا ينظر في عرض سعركم.
4. كفالة حسن تنفيذ بقيمة 10% من قيمة العطاء في حالة الترسية تأميناً نقدياً او كفالة بنكية او شيكاً مصدقاً سارية المفعول لمدة ثلاثة اشهر.
5. رسوم الاعلان على من يرسو عليه العطاء .
6. ضرورة الالتزام بالتسعير على النموذج المرفق بالعطاء .
7. ضرورة أن تكون الأجهزة المعروضة جديدة وليست مجددة .
8. يتم تقديم شهادة خصم مصدر في حالة تجاوز المبلغ قيمة 2500 شيكل او ما يعادلها.
9. غرامة تأخير 2% عن كل اسبوع وتبدأ من اليوم الذي يلي موعد التسليم المحدد من قبلكم، وفي حال تأخير التوريد مدة تزيد عن اسبوعين يحق للمستشفى إلغاء أمر الشراء والاحالة على مورد آخر وتحملكم فروق الأسعار.
10. الدفع خلال **90** يوماً من تاريخ الاستلام والفحص ومطابقة المواصفات الفنية المطلوبة .
11. تحديد فترة التسليم في عرض سعركم وايضاً فترة الضمان وأن تكون صلاحية العرض المقدم من طرفكم مدة لا تقل عن ثلاثة أشهر .
12. تسلم عروض الاسعار في مكتب مدير دائرة اللوازم والمشتريات رقم ( 6400 ) مبنى الإدارة في مستشفى النجاح الوطني الجامعي بالظرف المختوم فقط وتوضع في صندوق العطاءات ، على أن يكون عرض السعر يحوي فصلاً بين العرض المالي والعرض الفني أي أن العرض المالي منفصل عن العرض الفني مع ضرورة كتابة رقم العطاء على المغلفين وتوضيح اي منهما العرض الفني والعرض المالي.
13. على كل من يرغب بالمشاركة بتقديم عرض سعر تقديم ما لديه من مواد او اجهزة او ماركات لما جاء اعلاه او البديل له والرد على العطاء سلباً او ايجاباً .
14. يحق للمستشفى تجزئة العطاء وهي غير ملزمة بأقل الأسعار .
15. يحق للمستشفى إلغاء العطاء دون ابداء السبب ودون تحميل اية تكاليف مع اعادة رسوم نسخة العطاء للمشاركين في العطاء ان وجدت، ولا تتحمل المستشفى تكاليف النقل والتحميل والتنزيل .
16. ضرورة ارفاق الرخصة التجارية والسيرة الذاتية للشركة مع عرض السعر .
17. يرجى الالتزام بتعبئة كافة وثائق العطاء من صفحة 2 إلى صفحة 17 .
18. اخر موعد لتقديم عرض السعر هو يوم الخميس الموافق 2022-03-10 الساعة الواحدة ظهراً PM01:00 .
19. لأية إستفسارات متعلقة بالعطاء المذكور اعلاه ، يرجى الاتصال بالسيد مدير دائرة اللوازم والمشتريات هاتف رقم (97092389687) داخلي (6400) أو من خلال البريد الالكتروني tender3@najah.edu .

مدير دائرة اللوازم والمشتريات

إياد المكاوي



**طرح عطاء رقم – RFQ-H-11478**

**جدول الأسعار والكميات :**

No .	NNUH Code	Item	QTY	Unit	CODE #	وكيل / موزع	مدة التوريد	U.P (NIS)	T.P (NIS)
1	G-A-MDD00003	Patient monitor.	4	Pcs					
2	G-A-MDD00006	ECG machine.	2	Pcs					
3	G-A-MDD00019	Vital sign monitor	14	Pcs					
4	G-A-MDD00141	Central station monitor .	1	Pcs					
5	G-A-MDD00309	Defibrillator	2	Pcs					
6	G-A-MDD01204	Portable Patient monitor.	7	Pcs					
7	G-A-MDD01276	Fiberoptic Laryngoscope Curved with All blades size 0,1,2,3,4	2	Pcs					
8	G-A-MDF00013	Emergency trolley .	2	Pcs					
9	G-A-MDF00017	Stretcher	2	Pcs					
-	<b>Total Price (NIS)</b>								


*LM*



جدول المواصفات الفنية :

**ITEM 2**

OP06	Electrocardiograph (ECG), Qty: 2	Compliance Yes/No	Deviation
	<b>Good brand name with FDA or CE (Eurob, USA , Japan)</b>		
	Manufacturer:		
	Source and origin:		
	Model:		
	<b>Transport Stretcher, Specification:</b>		
	ECG Machine should have 8 inch Colour LCD Display.		
	The ECG Machine should be able to acquire all 12 Leads simultaneously and interpret them		
	Should acquire simultaneous 12 lead ECG for both adult and pediatric patients		
	Should have Real time Colour display of ECG waveforms with signal quality indication for each lead.		
	ECG machine should be installed on mobile trolley for transport.		
	Should have Artifact, AC, and low and high pass frequency filters.		
	Should have full screen preview of ECG report for quality assessment checks prior to print.		
	Should have interpretation facility of the amplitudes, durations and morphologies of ECG waveforms and associated rhythm for adult and pediatric patients.		
	Should have alphanumeric Keyboard for patient data Entry. (virtual or hard keys)		
	Should have High resolution (200 dpix500dpi on 25 mm/sec speed) digital array A4 size printer using thermal sensitive paper.		
	Should have battery capacity of at least 30 ECGs or 2 hours of battery backup.		
	Should be upgradable to be connected to HIS /LAN/Wireless LAN.		
	Should display ECG on LCD/TFT Display of 640x480 pixel resolution.		
	USB Support (optional) for Storage on external portable memories.		

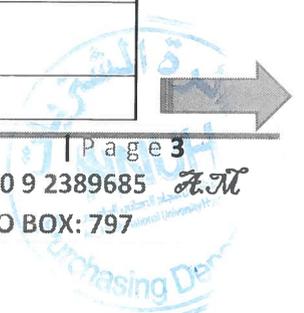


<b>Accessories &amp; consumables: to be included</b>		
10 Lead Patient Cable with Banana Plugs QTY 2		
Chest Electrodes Adult-(set of six) , 2 SETS		
Chest Electrodes Paediatric-(set of six), 2 SETS		
Limb Electrodes(set of 4), 2 SETS		
Thermal Paper A4 Size for 500 patients.		
Complete with all accessories and consumables needed to work completely as specified		
Your offer should contain the following: 1) Preventive maintenance schedual 2) Refernce list for the same model 3) Compliance sheet 4) Cataloges 5) Data sheet 6) Autherization latter 7) CE or FDA certificate 8) The service and operational manuals should delivered as soft copy with the units		

Warranty: 3 years, with commitment to conduct preventive maintenance (labor and parts) during the warranty period and according to manufacturer recommendations.



## ITEM 3

OP02	Vital sign monitor, Qty: 14	Compliance	Deviation
	<b>Good brand name with FDA or CE (Eurob, USA , Japan)</b>		
	Manufacturer:		
	Source and origin:		
	Model:		
	<b>Vital sign monitor Specification:</b>		
	Suitable for all types of Patient range: Adult, paediatric		
	Display- Touch screen minimum 8 inch		
	<b>NIBP Measurement:</b>		
	Technique: Oscillometric		
	Automatic Cuff Deflation		
	Accuracy : +/-5 mmHg and +/-2%BPM		
	Manual, STAT or Automatic (at preset intervals)		
	Auto Zero		
	Automatic measurement cycle adjustable		
	<b>SPO2 Measurement:</b>		
	Type: Functional Oxygen Saturation		
	Continuous Monitoring		
	Bar graph display of SpO2 signal strength		
	Accuracy :+/-3%		
	<b>Temperature Measurement:</b>		
	Predictive or Continuous Monitoring		
	Accuracy: +/-0.1°C		
	Parameters Displayed: Systolic Pressure, Diastolic Pressure and Mean Arterial Pressure (MAP),Pulse Rate,%SpO2, Temperature in Celsius,system status, plethysmogram, menus for user		
	Adjustable high and low alarms for Pulse Rate, SpO2, Systolic Pressure, Diastolic Pressure and Mean Arterial Pressure		
	Alarm Silence :Available		
	Memory :24hrs data storage		
	Battery : more than 3 hrs		
	<b>Each monitor should be supplied with the following Accessories:</b>		





1. NIBP: Adult (Qty. 2), pediatric (Qty. 1) cuff and hose		
2. Spo2 sensor: adult sensor with cable (Qty. 2), pediatric sensor with cable (Qty. 1).		
3. Temperature: Skin Temp. Probe (Qty. 2)		
4. vital sign monitor stand with basket		
Complete with all accessories and consumables needed to work completely as specified		
Your offer should contain the following: 1) Preventive maintenance schedual 2) Reference list for the same model 3) Compliance sheet 4) Cataloges 5) Data sheet 6) Autherization latter 7) CE or FDA certificate 8) The service and operational manuals should delivered as soft copy with the units		

Warranty: 3 years, with commitment to conduct preventive maintenance (labor and parts) during the warranty period and according to manufacturer recommendations.

**ITEM 1+4**

OP08+OP09	Patient monitor with central station, Qty: 4	Compliance	Deviation
OP02.1	Patient monitor, Qty: 4		
	<b>Good brand name with FDA or CE (Eurob, USA , Japan)</b>		
	Manufacturer:		
	Source and origin:		
	Model:		
	<b>Patient monitor Specification:</b>		
	Capable to monitor Adult and Pediatric Patients.		
	Monitor should have Touch screen user interface not less than 15 inch and with backup battery		
	Monitor Should be capable of 4 traces display		
	Facility to monitor and display ECG, Respiration ,NIBP, IBP SPO2, Temp, Heart rate and pulse		
	ECG should have capability for 3,5 and /or 10 lead monitoring and should have built in arrhythmia monitoring on all leads		
	Alarm limit status (On/Off) must be indicated on screen for each parameter and actual parameter alarm settings must be displayed on- screen when alarms are on.		
	Built in ST segment automatic & manual analysis		
	Position of the displayed waveforms must be user configurable		
	<b>Parameters:-</b>		
	<b>ECG and Respiration:</b>		
	Simultaneous multi-lead ECG (including 12 lead analysis) Respiration		
	Full lead select (I, II, III, aVR, aVL, aVF, and V (V1-V6 when using the ten lead cable) for display.		
	Each monitor simultaneously obtains, at minimum, three ECG leads for QRS detection and arrhythmia recognition.		
	Trace Sweep Speed 50,25,12.5-mm/sec		
	Respiratory signal is obtained through the ECG leads.		
	Pace maker pulse rejection		

The user can select Lead I or Lead II for respiratory cycle monitoring and waveform display.		
The respiration program includes the following features:		
Manual and automatic waveform sizing.		
Auto and manual respiratory cycle threshold detection.		
The system has adjustable alarm settings for high and low respiration rate and Apnea.		
ECG trend must be beat-to-beat		
Defibrillator and ESU protection provided		
Patient leakage current, less than 10uA		
<b>NIBP: 1-channel</b>		
Measurement modes include: Manual mode		
The monitor displays systolic, diastolic, mean values, and time of pressure determination. (In timed auto mode, display shows time to next reading.)		
Measurements are tabulated for recall and review.		
<b>IBP: 2- Channel</b>		
The monitor should be capable of displaying the waveforms at different speeds		
The monitor automatically measures the PAW.		
Alarm Limit Adjust high and low limit		
<b>Temp: 2- Channel</b>		
Measurement Range : 0 to 50°C		
Numeric up to date Rate: every 3 sec.		
Alarm limit adjustable high and low limits		
<b>Pulse Oximetry:</b>		
The monitor can measure oxygen saturation using pulse oximetry.		
The module offers compatibility with two or more probe manufacturers.		
The user can select the SpO2 waveform for display.		
The monitor displays an O2 saturation value and a pulse		
The SpO2 program includes the following features: High and low alarm limits for O2 saturation Automatic waveform sizing		
Signal strength indicator		

	Displayed messages include: Interference detected, low light, check probe, low signal quality, probe off patient, replace probe.		
	<b>Each monitor should be supplied with the following Accessories:</b>		
	1. ECG/Respiration: 5 lead ECG cable with clip (Qty.2 sets)		
	2. NIBP: Adult (Qty. 2), pediatric (Qty. 1) cuff and hose		
	3. Spo2 sensor: adult sensor with cable (Qty. 2), pediatric sensor with cable (Qty. 1).		
	4. Temperature: Skin Temp. Probe (Qty. 2)		
	5. IBP kitt (Qty. 1)		
	6. CGX with height and tilt mounting solution for all monitors included.		
	Complete with all accessories and consumables needed to work completely as specified		
	<b>Should be compatible with the central station</b>		
OP02.2	<b>Central station, Qty: 1</b>		
	<b>Good brand name (Eurob, USA , Japan)</b>		
	Manufacturer:		
	Source and origin:		
	Model:		
	<b>Central station Specification:</b>		
	Central station should have min 17 inch high resolution color display		
	System should have minimum 8 beds monitoring capability		
	Automatic data save in case of power failure		
	It should have possible to view information such as vital sign ,alarm status , arrhythmia analysis ,tendered parameter, patient data etc , for any selected bed from the central station.		

Displayed information: Access to complete patient information including alarm histories, graphic trends, tabular vital signs, and one hour Full Disclosure		
Instantaneous access to all patient monitoring information		
multiple patient view : continuously view up to 4 waveforms for up to 8 patients		
Should have default alarm limits and customizable parameter settings, Interactive alarm display ,Color-coded alarm notification, alarm silencing for 1 min.		
1TB Hard drives at least		
Support of HL7 protocol		
Key board, mouse ,are included		
<b>Should be compatible with the patient monitors</b>		
Your offer should contain the following: 1) Preventive maintenance schedual 2) Refernce list for the same model 3) Compliance sheet 4) Cataloges 5) Data sheet 6) Autherization latter 7) CE or FDA certificate 8) The service and operational manuals should delivered as soft copy with the units		

Warranty: 3 years, with commitment to conduct preventive maintenance (labor and parts) during the warranty period and according to manufacturer recommendations.

**ITEM 5**

OP03	Defibrillator, Qty: 2	Compliance	Deviation
	Good brand name with FDA or CE (Eurob, USA , Japan)		
	Manufacturer:		
	Source and origin:		
	Model:		
	<b>Defibrillator Specification:</b>		
	Biphasic, Manual and AED		
	Energy selection 5 J to 200 J or above in steps		
	Momentary energy selection access on front panel.		
	Should have adult and pediatric paddles integrated on same handle		
	Charge key on front panel and on the apex hand.		
	Monitor should display selected and delivered energy		
	Should have pacing and synchronization mode		
	Energy should be delivered within 30ms after the detected R wave in synchronization mode.		
	Should have battery back up for 50 discharges of 200J.		
	Should have ECG inputs		
	Should have display for selected ECG input source(I, II, III, paddles)		
	Amplitude gain of ECG waveform should be adjustable		
	Should have alarm for high and low HR with a provision for alarm silence mode		
	Should have an inbuilt thermal recorder.		
	Should have enable/disable option for printer.		
	Should Supply along with placing cable with pad.		
	Complete with all accessories and consumables needed to work completely as specified		




Your offer should contain the following:

- 1) Preventive maintenance schedual
- 2) Refernce list for the same model
- 3) Compliance sheet
- 4) Cataloges
- 5) Data sheet
- 6) Autherization latter
- 7) CE or FDA certificate
- 8) The service and operational manuals should delivered as soft copy with the units

Warranty: 3 years, with commitment to conduct preventive maintenance (labor and parts) during the warranty period and according to manufacturer recommendations.

**ITEM 6**

OP01	Portable patient monitor, Qty: 7	Compliance	Deviation
	<b>Good brand name with FDA or CE (Eurob, USA , Japan)</b>		
	Manufacturer:		
	Source and origin:		
	Model:		
	<b>Portable patient monitor Specification:</b>		
	Can be hooked to patient transfer trolley or stand		
	Battery operated with run time not less than 3 Hrs		
	Alarms : visual and audible		
	touch screen display not less than 9 inch		
	<b>Parameter for the patient monitor mentioned in point OP02.1</b>		
	<b>Each monitor should be supplied with the following Accessories:</b>		
	1. ECG/Respiration: 5 lead ECG cable with clip (Qty.2 sets)		
	2. NIBP: Adult (Qty. 2), pediatric (Qty. 1) cuff and hose		
	3. Spo2 sensor: adult sensor with cable (Qty. 2), pediatric sensor with cable (Qty. 1).		
	4. Temperature: Skin Temp. Probe (Qty. 2)		
	5. IBP kitt (Qty. 1)		
	6. Monitor stand with counter weight		

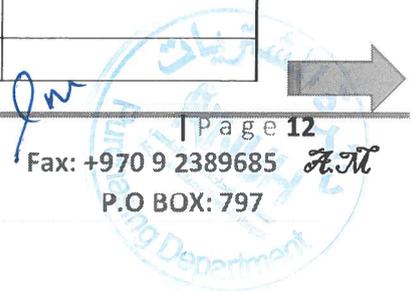

Complete with all accessories and consumables needed to work completely as specified		
Your offer should contain the following: 1) Preventive maintenance schedual 2) Reference list for the same model 3) Compliance sheet 4) Cataloges 5) Data sheet 6) Autherization latter 7) CE or FDA certificate 8) The service and operational manuals should delivered as soft copy with the units		

Warranty: 3 years, with commitment to conduct preventive maintenance (labor and parts) during the warranty period and according to manufacturer recommendations.


**ITEM 7**

OP05	Fiber optic laryngoscope , Qty: 2	Compliance	Deviation
	Good brand name		
	Manufacturer:		
	Source and origin:		
	Model:		
	<b>Fiber optic laryngoscope Specification:</b>		
	Fiber optic Laryngoscope from reputable manufacturer with all blades size		
	Your offer should contain the following: 1) Preventive maintenance schedual 2) Reference list for the same model 3) Compliance sheet 4) Cataloges 5) Data sheet 6) Autherization latter 7) CE or FDA certificate 8) The service and operational manuals should delivered as soft copy with the units		

Warranty: 1 years

**ITEM 8**

OP04	Emergency Trolley , Qty: 2	Compliance	Deviation
	Good brand name		
	Manufacturer:		
	Source and origin:		
	Model:		
	<b>Emergency Trolley Specification:</b>		
	Backboard		
	Iv pole holder		
	Two small drawers with partitions		
	One large drawer		
	Defibrillator swing arm		
	Lockable drawer for dangerous drugs		
	Mobile on 4 castors with break mechanism		
	Oxygen tank holder		
	Drawer cassette for top cavity		
	<b>Each trolley should be supplied with the following Accessories:</b>		
	O2 cylinder complete with regulator flow meter and mask		
	Diagnostic set		
	Fully catheters 8 sizes 10 each		
	Ambo bag set silicon child, adult		
	Dressing set (specify)		
	Endotrachial tube 8 sizes 10 each		
	Complete with all accessories and consumables needed to work completely as specified		
	<b>OPTIONAL TO BE PRICED SEPARATELY:-</b>		
	O2 cylinder complete with regulator flow meter and mask		
	Diagnostic set		
	Fully catheters all sizes ( 10 for each size)		
	Ambo bag set silicon infant, child, adult		
	Dressing set (specify)		
	Endotrachial tube all sizes (10 for each size )		

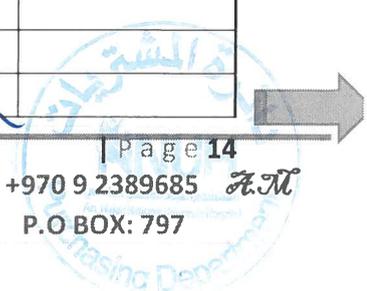



Your offer should contain the following:

- 1) Preventive maintenance schedual
- 2) Refernce list for the same model
- 3) Compliance sheet
- 4) Cataloges
- 5) Data sheet
- 6) Autherization latter
- 7) CE or FDA certificate
- 8) The service and operational manuals should delivered as soft copy with the units

Warranty: 1 years



**ITEM 9**

OP7	Transport Stretcher, Qty: 2	Compliance Yes/No	Deviation
	<b>Good brand name with FDA or CE (Eurob, USA , Japan)</b>		
	Manufacturer:		
	Source and origin:		
	Model:		
	<b>Transport Stretcher, Specification:</b>		
	To be used in emergency , recovery and for patient transfer		
	Should have pneumatic stepless adjustment for back section, Trendelenburg , reverses trendelenburge , and foot section.		
	Should have hydraulic height adjustment from both sides of the trolley.		
	Should have central braking system with steering facility.		
	Should be equipped with heavy duty castors		
	Should have bumpers at all the four corners and middle of the mattress base frame.		
	Should have handle for transportation		
	Should have place for fixing oxygen cylinder.		
	Weight capacity not less than 200 Kg.		
	Dimensions:		
	1- Max length not less than 2000 mm		
	2- Max width not less than 750 mm		
	3- Height adjustable 550 – 900 mm approx.		
	4- Trendelenburg up to 20 deg stepless.		
	5- Reverse Trendelenburg up to 10 deg stepless.		
	<b>Accessories &amp; consumables: to be included</b>		
	Anti static hygienic mattress , 80mm with pull straps.		
	Side Rails from both sides.		



IV rod qty 2		
foot end panel		
Complete with all accessories and consumables needed to work completely as specified		
Your offer should contain the following: 1) Previntive maintenance schedual 2) Refernce list for the same model 3) Compliance sheet 4) Cataloges 5) Data sheet 6) Autherization latter 7) CE or FDA certificate 8) The service and operational manuals should delivered as soft copy with the units		

Warranty: 3 years

Finish

يرجى الإلتزام بتعبئة الجدول التالي :

	إسم الشركة	1
	الختم	2
	التوقيع والإسم	3
	معلومات الإتصال	4
	مدة التوريد	5
	مدة الكفالة إن وجدت	6